Transition to **Micro**Doc® sNPWT Decision Tree

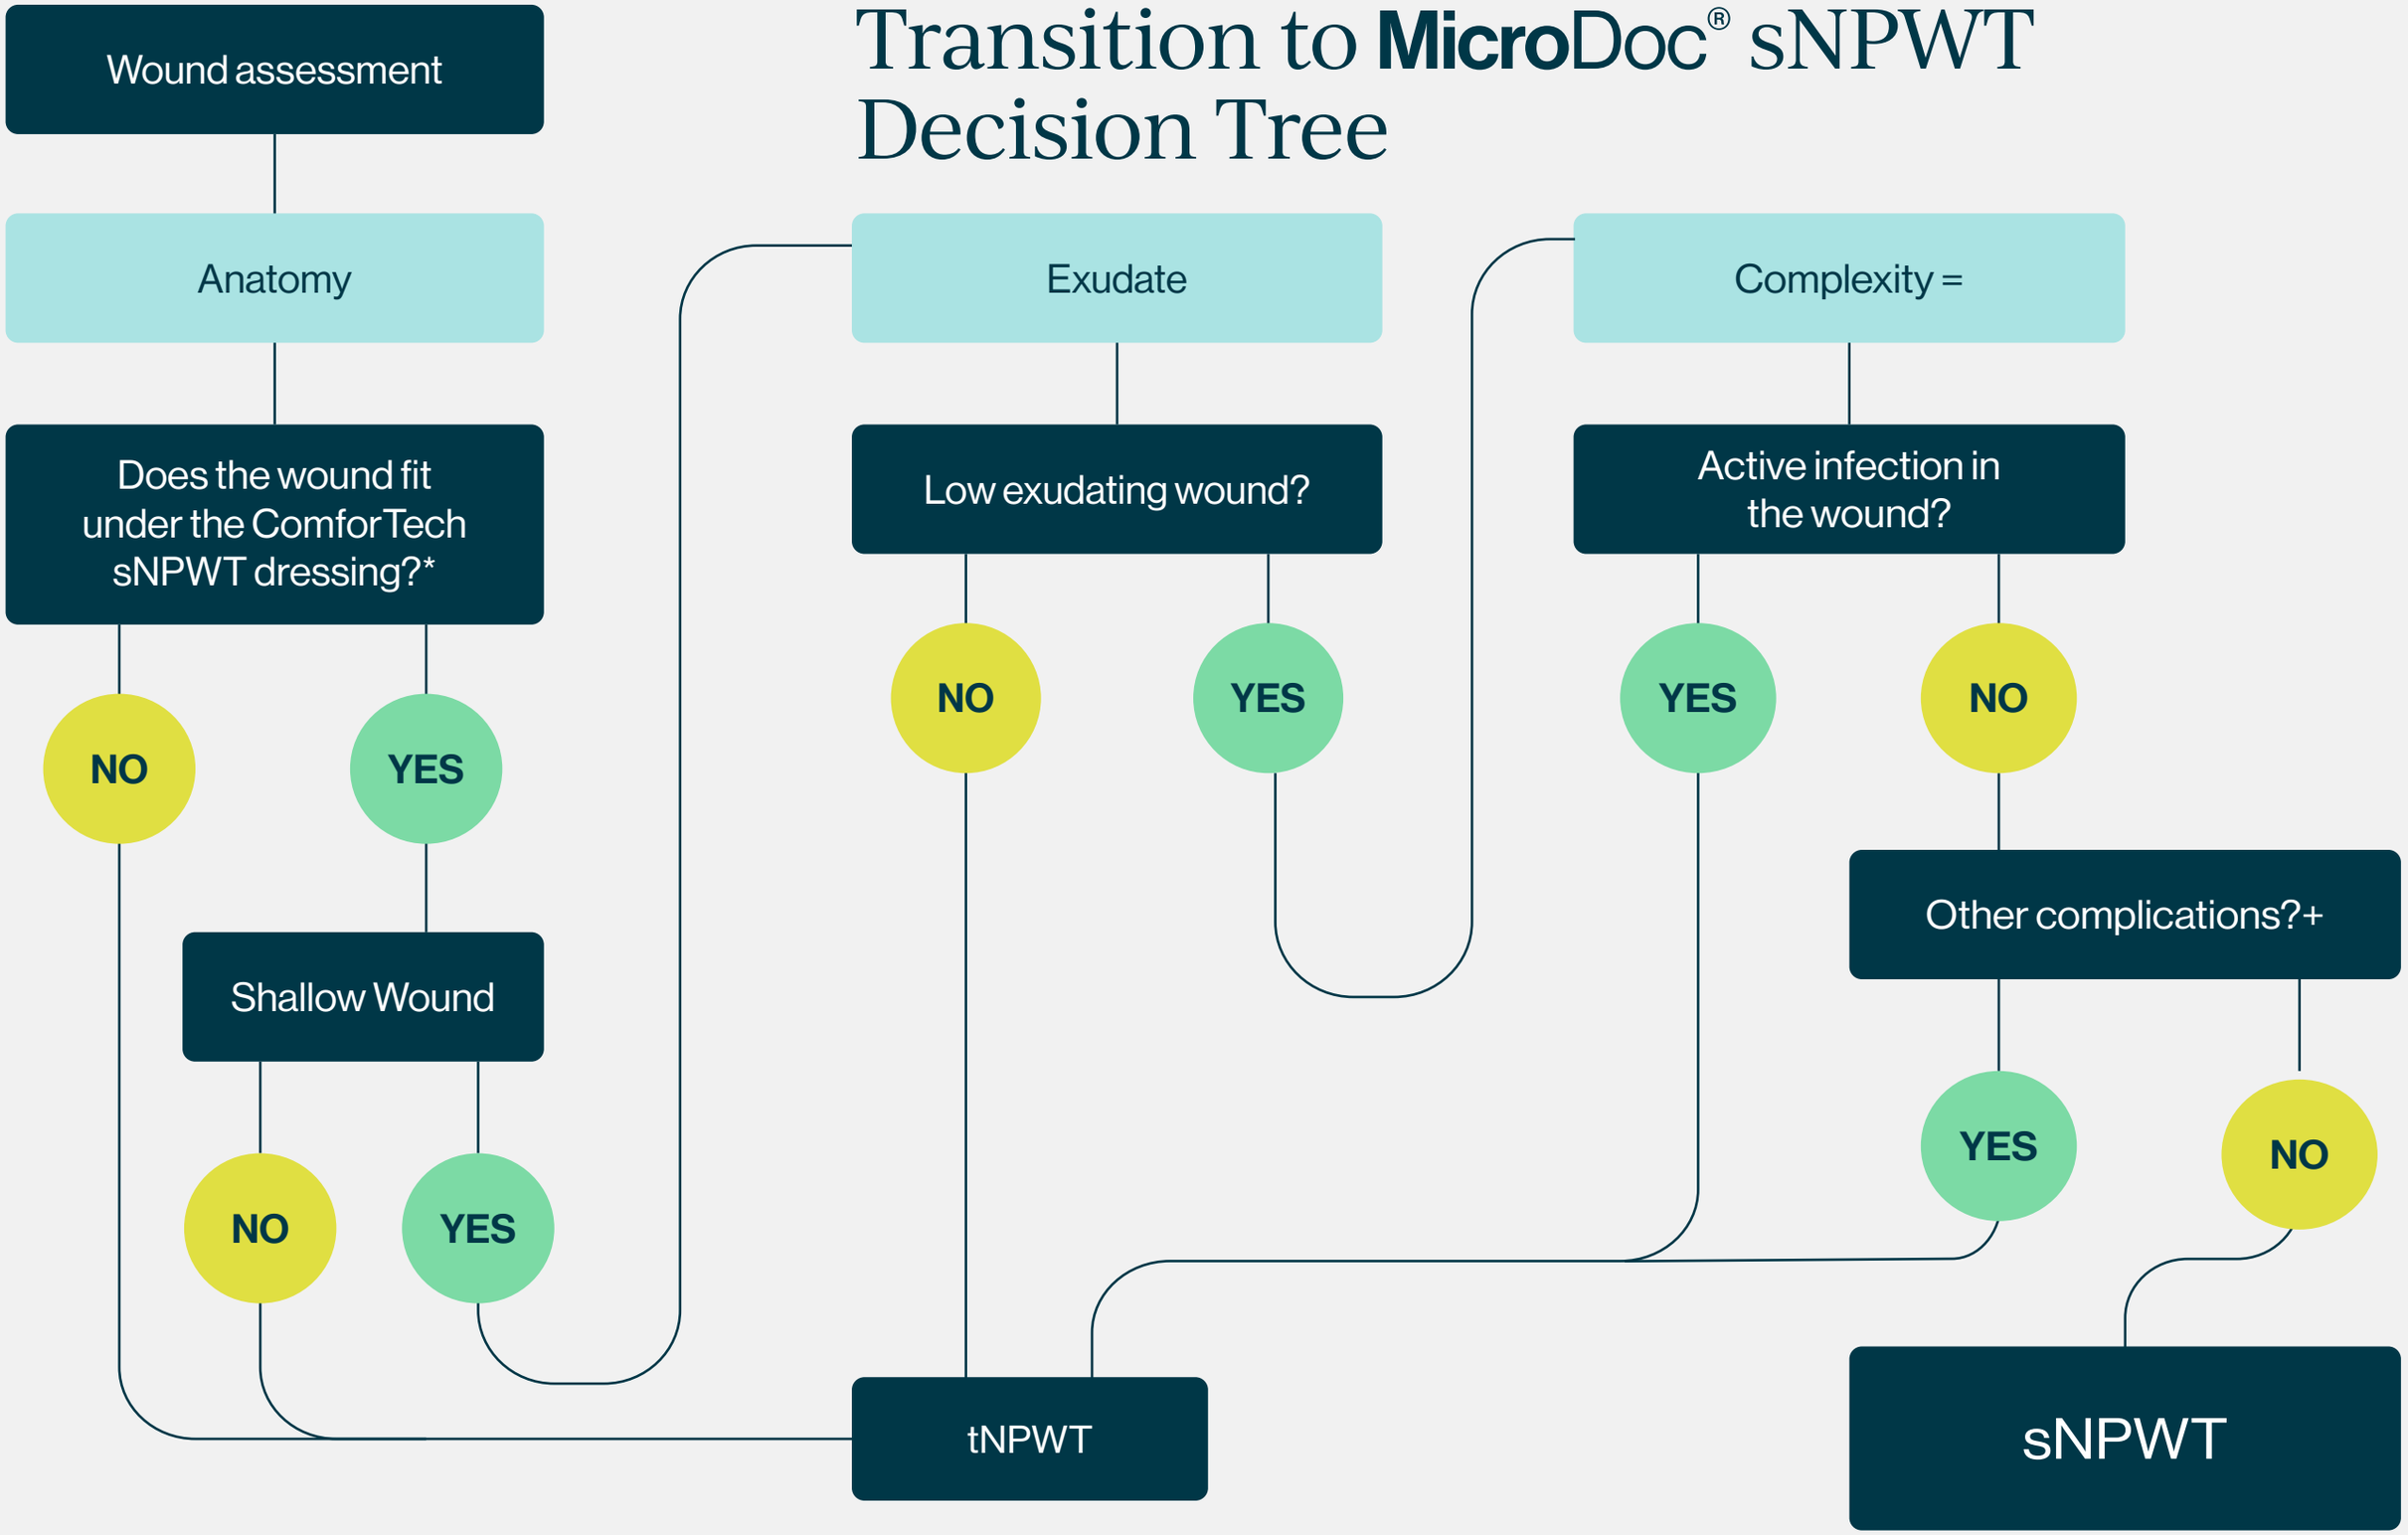

* Anatomical locations should be assessed for sNPWT appropriateness (e.g. amputations, sacral wounds, etc).
= Degree of complexities should be assessed individually to promote positive outcomes when implementing sNPWT.
+ Complications prohibiting sNPWT e.g. Seroma, hematoma, numbness, cool to touch, dehiscence, poor pallor, etc.

Pensar Medical™

The Pensar Medical products are medical devices and must be used in strict adherence to the Operator's Manual; failure to do so may result in serious personal injury. It is strongly recommended that you regularly consult Pensar Medical website (www.pensarmedical.com) for the latest available information. Please contact Pensar Medical should you have any questions. Use only under the supervision of qualified medical personnel. Consult the Operator's Manual and Pensar Medical website (www.pensarmedical.com) for appropriate product designation. Failure to obtain and follow the recommendations of your medical care provider may result in serious personal injury.